

PERFORMANCE OF THE ADVANCED PHOTON SOURCE (APS) LINAC BEAM POSITION MONITORS (BPMs) WITH LOGARITHMIC AMPLIFIER ELECTRONICS*

R. E. Fuja and M. White

Argonne National Laboratory, 9700 S. Cass Avenue, Argonne, IL 60439 USA

Abstract

This paper discusses the performance of the logarithmic amplifier electronics system used with stripline BPMs to measure electron and positron beam positions at the APS linac. The 2856-MHz, S-band linac accelerates 30-nsec pulses of 1.7 A of electrons to 200 MeV, and focuses them onto a positron conversion target. The resulting 8 mA of positrons are further accelerated to 450 MeV by the positron linac. Beam position resolutions of 50 μm are easily obtainable in both the electron and positron linacs. The resolution of the 12-bit A/D converters limits the ultimate beam positron resolution to between 20 and 30 μm at this time.

I. INTRODUCTION

The APS linac BPM system, in operation for over a year, has been used in the commissioning of both the 200-MeV electron and the 450-MeV positron beams. It consists of stripline pickups and signal processing electronics using logarithmic amplifiers. The system has proven very reliable with only one problem occurring in an A/D section. System stability has not been a problem, and beam can be transported to the end of the linac a few minutes after being turned on.

II. EXPERIMENT

The following data were taken to determine the resolution of the linac BPM system in the presence of pulsed power supply noise. Background on the detectors and the processing electronics is provided.

A. Detectors

Stripline-type BPMs [1], were chosen because they provide -5 dBm of peak signal from the 8-mA positron beam. The BPMs are cylindrical in geometry, and the four striplines are mounted 90 degrees apart. The striplines are 1 inch long and subtend an arc of 1 radian. Their geometry is such that they form 50-Ohm pickups. The measured electrical length of the striplines is 0.21 wavelengths at 2.856 GHz. The average detector sensitivity is 1.73 dB/mm \pm 0.1 dB. Signals from the striplines are transported via 1/4-inch heliax cable to electronics located an average of 85 feet away in the klystron gallery. About 10 dB of signal is lost over this distance.

* Work supported by U.S. Department of Energy, Office of Basic Energy Sciences, under Contract No. W-31-109-ENG-38.

Five BPMs are installed in the electron linac, one downstream of each accelerating structure, and seven BPMs are installed in the positron linac, one downstream of each of the last seven accelerating structures. There are no BPMs downstream of the first two accelerating structures after the target in the positron linac.

B. Electronics

The electronics [2], can be subdivided into two sections, a downconverter section and a logarithmic amplifier section. The downconverter section consists of a 2.856-GHz to 70-MHz downconverter followed by a 70-MHz bandpass filter and amplifier. The bandpass filter stretches the 30-nsec pulse to around 200 nsec and reduces its amplitude by some 13 dB. The overall gain of the downconverter is around 6.2 dB and it has a noise figure of around 7.5 dB. This 70-MHz signal is used as the input to a cascaded chain of logarithmic amplifiers consisting of two Analog Devices AD640s with their video bandwidths set to 7 MHz. The input power to the logarithmic amplifiers is adjusted to -10 dBm for the two different beam intensities in the electron and positron linacs. The sensitivity of the logarithmic amplifier chain is 53 mV/dB \pm 1 mV. The calibration shown in Figure 1 is typical of all logarithmic amplifier sections.

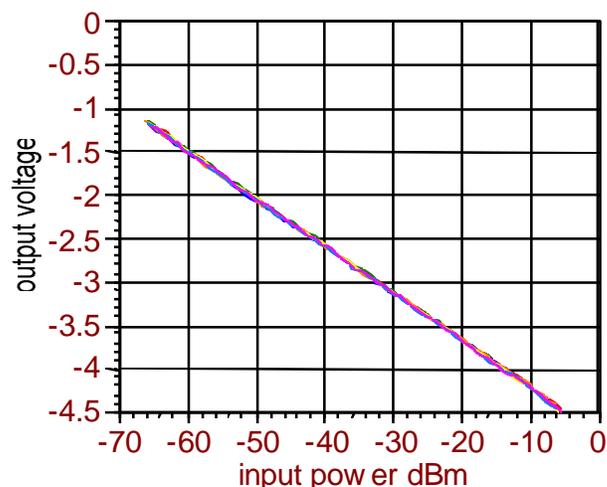


Figure 1: Dynamic ranges of eight different logarithmic amplifier channels. The slope is -54.26 ± 0.6 mV/dBm, and the intercept is at -4.756 ± 0.02 V.

Eight logarithmic amplifier channels are mounted on a single VXI card and process the signals from two BPMs. The VXI card also contains eight sample and hold circuits and eight 12-bit analog-to-digital converters. A specially designed VXI trigger module [3] contains a set of 8-bit programmable delay lines that can be used to select sample times in increments of 5 nsec. Software peak detection by scanning is available for all BPM signals, replacing the more commonly used peak detection circuits.

With a detector sensitivity of 1.73 dB/mm and a logarithmic amplifier sensitivity of 53.3 mV/dB the overall sensitivity of the system becomes 94 mV/mm. The gain of each downconverter channel was adjusted by injecting a 2.856-GHz signal into the cable at the detector end and adjusting the amplitude of the 70-MHz output. Phase shifters at the input to the downconverter enabled the phase between two 70-MHz output signals to be matched. Zeroing the phase shifts was necessary because of coherent noise in the system; 5 mV corresponds to 53 μ m. The signal difference for two typical channels is shown in Figure 2.

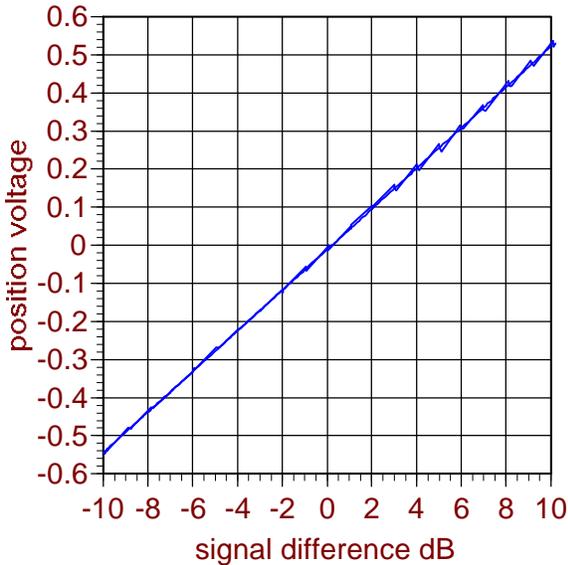


Figure 2: Signal difference between 2 channels for input power levels of -15, -25, and -35 dBm. The slope is 53.31 mV/dB and the offset is -10.2 mV.

III. RESULTS

The results presented below were obtained during a positron studies run and they are the best to date. Typically, operating conditions result in data from selective positron linac BPMs that are up to five times worse. Electron linac BPMs consistently provide good data because the signals are large. The results from positron linac BPMs vary because both electrons and positrons are present in a ratio that depends on the particular transport optimization at the time. The amplitude of the signal they receive depends on the

magnitude of the charge difference between electrons and positrons. The charge of the particle that is present in excess is unknown and must be determined by other means. Figure 3 shows data taken from the BPM located just upstream of the positron target, when 1.06 A of electrons were hitting the target. With 16 samples, the standard deviation of the readings from individual electrodes is 5 to 7 mV and the standard deviation in the difference of two signals is 1 to 2 mV, corresponding to 21.3 μ m. Figure 4 shows BPM data from the detector furthest downstream in the positron linac. Here the intensity reading is 6 mA and represents the magnitude of the sum of the positron and electron currents in the beam. Other measurements made in the low energy transport line after a bending magnet indicate that 4 mA of positrons were present at that time. Here the standard deviation in the position measurement is 3 mV or 33 μ m.

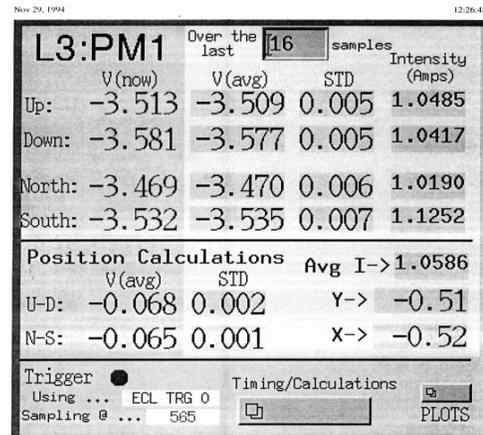


Figure 3: Data taken from the BPM located just upstream of the positron target, when 1.06 A of electrons were hitting the target.

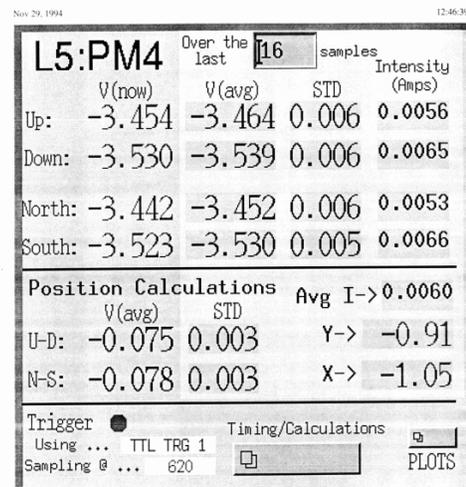


Figure 4: BPM data from the last detector in the positron linac. Here the intensity reading is 6 mA, the magnitude of the sum of the positron and electron currents.

IV. CONCLUSION

With proper phasing of the stripline signals it is not difficult to obtain the results shown. With the signal-to-noise ratio at the input to the logarithmic amplifier circuits approaching 75 dB, resolutions of 1 μm should be possible.

A new BPM system that gives information on the polarity of the charged particle producing the signal (electron or positron) has been worked out, and will provide for much improved positron diagnostics capability [4]. A prototype is under development.

V. ACKNOWLEDGEMENTS

The authors would like to thank C. Gold for his help in the laboratory and in the installation, J. Stephens for his help with the software testing programs, and N. Arnold and K. Ko for developing the control systems and operating screens.

VI. REFERENCES

- [1] R. Shafer, "Beam Position Monitoring," Accelerator Instrumentation, Upton, N.Y., 1989, *AIP Conference Proceedings 212*, pp. 26-58, (1989).
- [2] R. Fuja and Y. Chung, "The APS Linac Beam Position Monitor and Electronics," Proc. of the 4th Accel. Instr. Workshop, Berkeley, CA., October 1992, *AIP Conference Proceedings No. 281*, pp. 248-255 (1993).
- [3] A.E. Grelick, private communication.
- [4] W. Sellyey, private communication.